

# Aqua Rite & Aqua Rite XL

## Diagnositics Manual



## Turbo Cell & Control Electronics

Software Revision 1.50

# Table of Contents

Important safety instructions	Pg. 1
Check Salt/Inspect Cell LED flashing or ON	Pg. 2-3
How to Set Cell Type	Pg. 4
How to Reset Average Salt Level	Pg. 5
Adjusting Chlorine Output	Pg. 6
High Salt LED ON	Pg. 7
No Flow LED flashing or ON	Pg. 8
No LED's/LCD display	Pg. 9-12
Low/High Cell temperature	Pg. 13
Cell cleaning instructions	Pg. 14-16
Troubleshooting flow charts	Pg. 17-21
Salt Chart	Pg. 22
Software Revision Compatibility Chart	Pg. 23
Important Information- Chlorine output and salt	Pg. 24

# Aqua Rite/Aqua Rite XL Diagnostics




## High Voltage Electrocution Hazard

Hazardous voltage can shock, burn, cause serious injury and or death. To reduce the risk of electrocution and or electric shock hazards:

- Only qualified technicians should remove the panel
- Replace damaged wiring immediately
- Insure panel is properly grounded and bonded

# Check Salt & Inspect Cell LED flashing or ON

**Check Salt & Inspect Cell LED's will flash together when salt level is between 2500-2600ppm. Chlorine is still being produced. Check Salt & Inspect Cell LED's will be ON when salt level is 2300ppm or less. Chlorine production is halted. Inspect Cell LED will flash by itself when 500 operational hour countdown timer has expired. Requires manual reset. To manually reset the Inspect Cell LED, press and hold the Diagnostics button until LED goes out (approximately 3 to 5 seconds).**

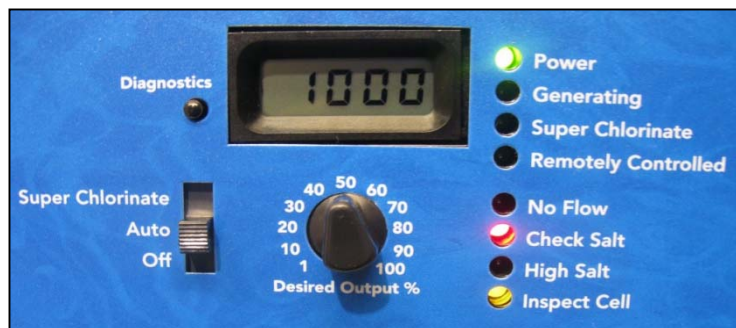

**NOTE: Check Salt & Inspect Cell LED's will also be ON if the control is set for the wrong Turbo Cell type or the cell is unplugged.**

Step A


**Verify salt level is 2700-3400ppm and check with independent test to ensure accuracy. 3200ppm is the ideal level.**



**If salt level is within range, go to step B.  
If salt level is below range, add enough salt to achieve a salt level of 3200ppm.  
(Refer to Salt Chart, Page 21)**

Step B

**Inspect and/or Clean Cell**

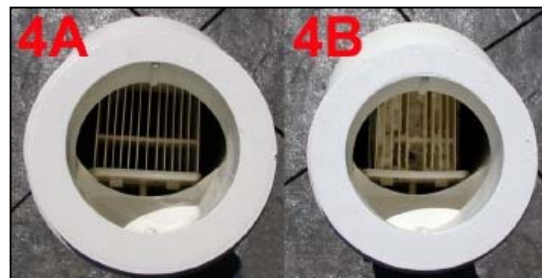

**If cell looks like 4A, go to step C.  
If cell looks like 4B, clean cell.  
(Refer to Pages 12 thru 15)**

# Check Salt & Inspect Cell LED flashing or ON

Check cell voltage and amperage in both polarities.




Step C



Voltage Range: 22.0 – 26.0 VDC



T-15 Amp Range: 3.1 – 8.0 amps  
T- 9 Amp Range: 2.3 – 6.7 amps  
T-5 Amp Range: 1.9 – 5.7 amps  
T-3 Amp Range: 1.3 – 4.5 amps

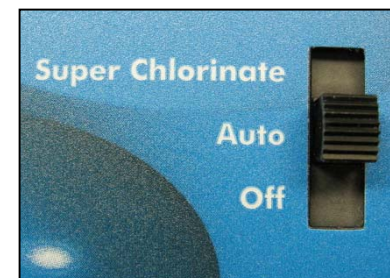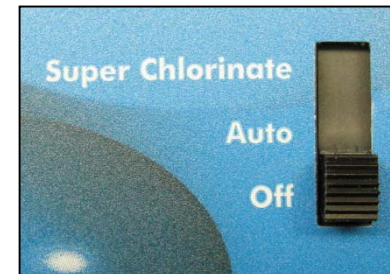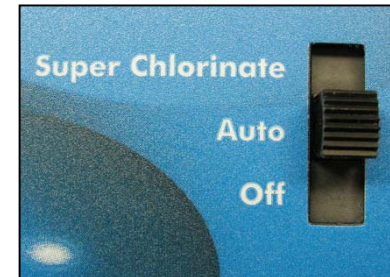

To switch polarities, cycle Main Switch from  
AUTO → OFF → AUTO.




# How To Set Turbo Cell Type

Before operation, the Aqua Rite must be configured for the chlorinator cell that will be used. "t-15" is the factory default. If the incorrect cell is chosen the salt level, amperage, and voltage will not be correct and the system will turn the chlorinator off.


Slide the Main Switch to the "Auto" position.



To switch Cell Type, cycle Main Switch from AUTO → Super Chlorinate → AUTO.

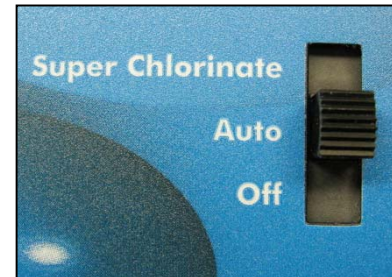

Push the diagnostic button until "t-xx" appears on the display.

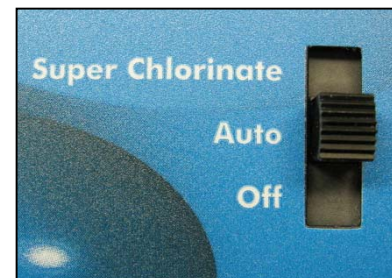

# How to Reset Average Salt Level

The Average Salt level needs to be reset for start up and when a cell is replaced. (factory default is 2800ppm)

To reset, turn the unit to Off and then back to Auto. Wait for the relay to click (5 to 10 seconds).



Press Diagnostics button 5 times to display Instant Salt level. Wait for the number to settle.



Cycle slide Main Switch from Auto → Super Chlorinate → Auto


# Adjusting Chlorine Output

## Desired Output % Dial

1 to 100% sets the level of cell operation in % of operating time..

Example: 50% (factory default) cell is operating and generating chlorine 50% of the total pump/filter operating time.

Refer to page 24 for important additional information !

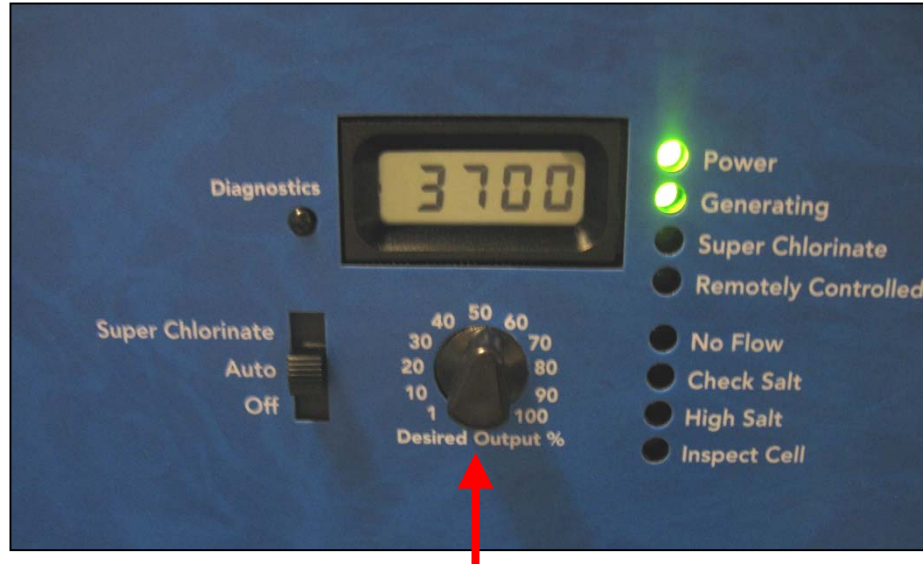

Rotate the dial to adjust.

*Note: If the chlorine level does not increase within 24 hours after increasing output, test water with independent tests to determine current salt, stabilizer, phosphate, and nitrate levels.*

*Note: Output is scaled back to 20% of desired output setting at 60° F and output stops at 50° F.*



# High Salt LED ON

*The High Salt LED will be ON when the cell amperage is above the maximum limit. High Salt LED will also be ON if the control is set for the wrong Turbo Cell type.  
The LCD display will read "HI".*

**Verify salt level is 2700-3400ppm and check with independent test to ensure accuracy.**



**Maximum Current (Amps) before shutdown**

T-Cell 3: 4.15

T Cell 9: 9.50

T-Cell 5: 6.40

T Cell 15: 10.00


If salt level is above the range, partially drain pool and/or spa and refill with fresh water to achieve a salt level of 3200ppm.

( RULE of THUMB: Each inch of water drained will reduce the salt level 100ppm.)

# No Flow LED flashing or ON

*No Flow LED will flash for up to 60 seconds on start-up.*

*No Flow LED will be ON when there is a flow switch problem.*

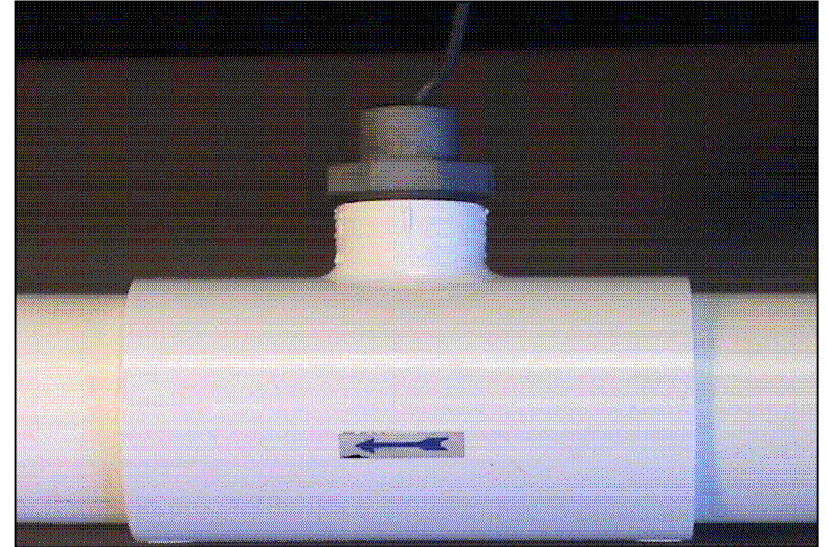




If LED is flashing, wait 60 seconds after starting filter pump. Check for possible turbulence inside of flow T. Installation requires 12 inches of straight pipe before flow switch. There should be no elbow after the flow switch.

If LED is ON, check for flow switch installed backward. Arrows at the top of the hex nut need to point in the direction of water flow. Flow switch requires a minimum flow rate of 11 gpm to stay closed consistently. Check for damaged or cut wire.



# No LED's/LCD display


Verify 220-240 VAC or 115-125 VAC  
at input terminal TB1.

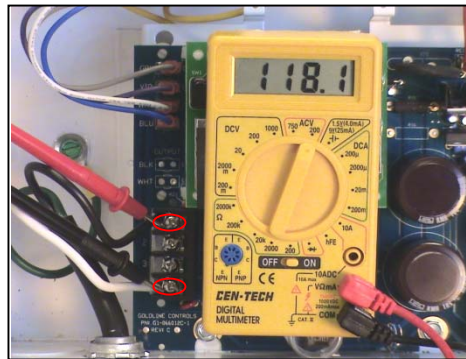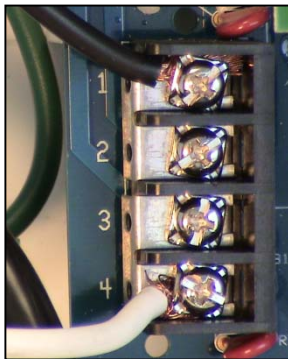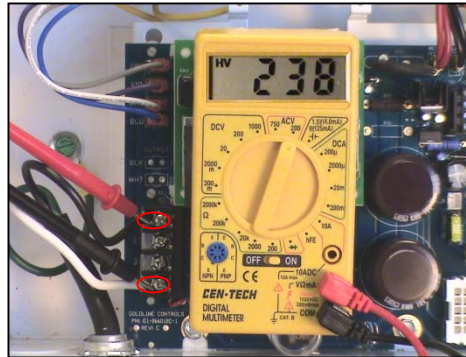

If voltage is good, go to step D.  
If no voltage, check to see that breaker  
and/or time clock are not off.  
Check input jumpers for correct position.  
220-240 VAC: jumpers on 2 & 3 (factory default)  
115-125 VAC: jumpers on 1 & 2 and 3 & 4

Step D

Verify 20-24 VAC  
between yellow wires


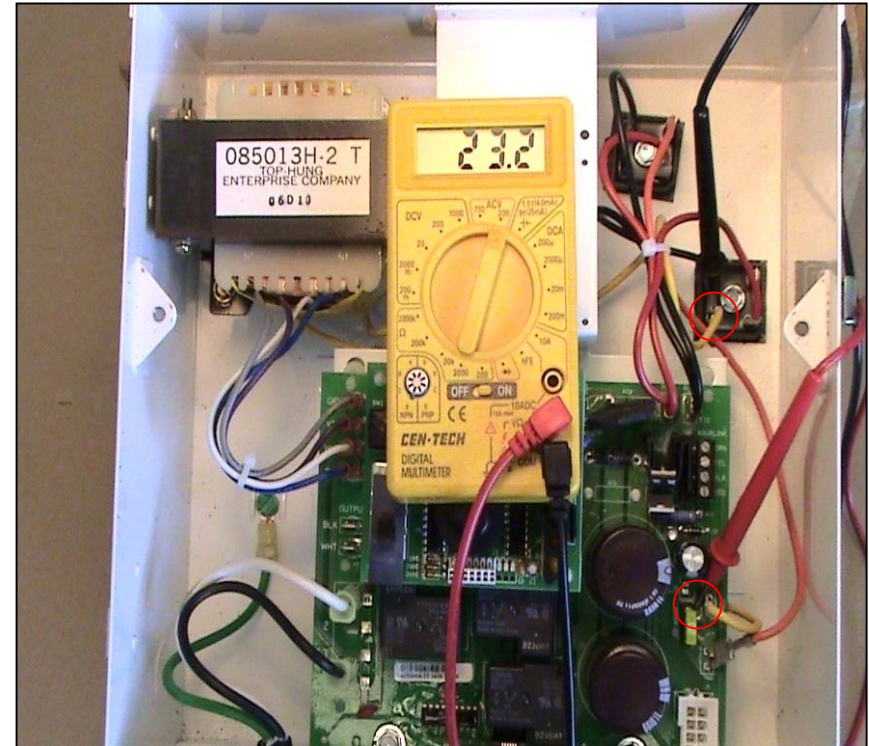


If no voltage go to step E.  
If voltage is good go to step F.

# No LED's/LCD display

**Shut off power to the control box.  
Disconnect the blue, white, gray and  
violet wires from the main board and  
measure the following:**

Step E

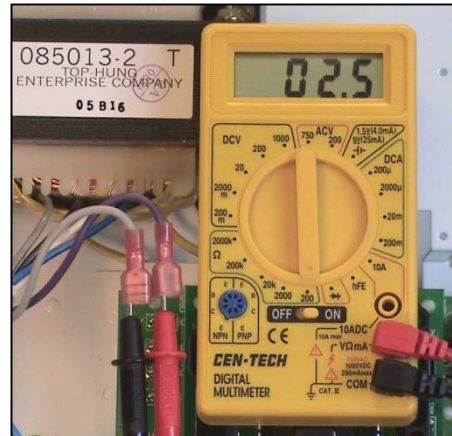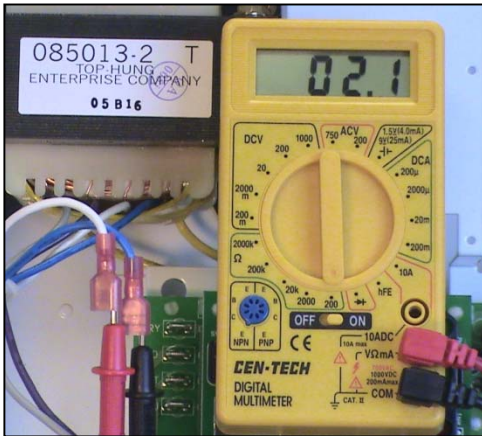


**Insert probes and measure resistance between the  
Blue & White wires and the Violet & Gray wires.  
The readings should be 2.0- 2.9 Ohms.**

**If the readings of either of the two measurements are not  
2.0 – 2.9 Ohms, the transformer is faulty and should be replaced.  
If measurements are OK, go to step F.**

**Test for continuity of  
20 amp slow blow fuse**

Step F

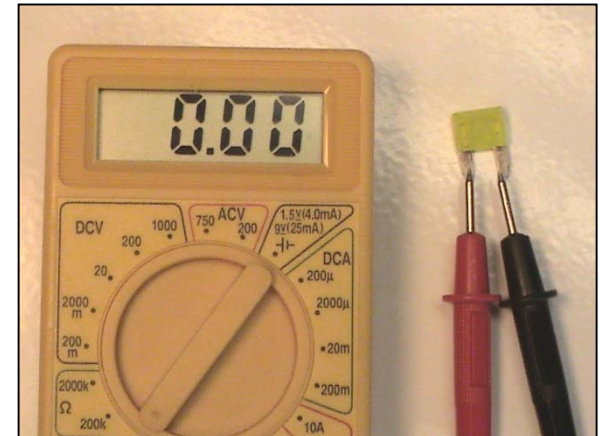


**Replace fuse if blown. If fuse OK, go to step G.**



# No LED's/LCD display

**Verify 18-33 VDC between black & red wires on main board**


Step G

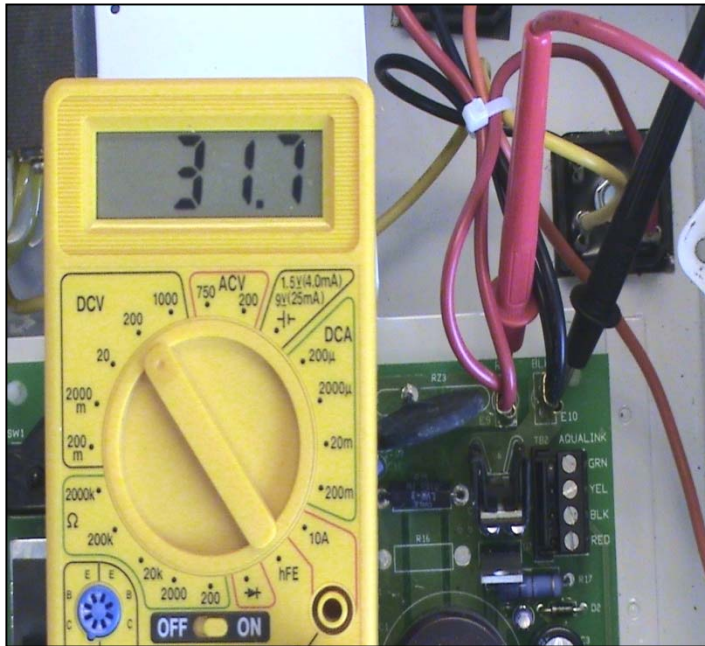

**If no/low voltage replace rectifiers.  
If voltage OK, go to step H.**

**Reseat DSP Board**

Step H

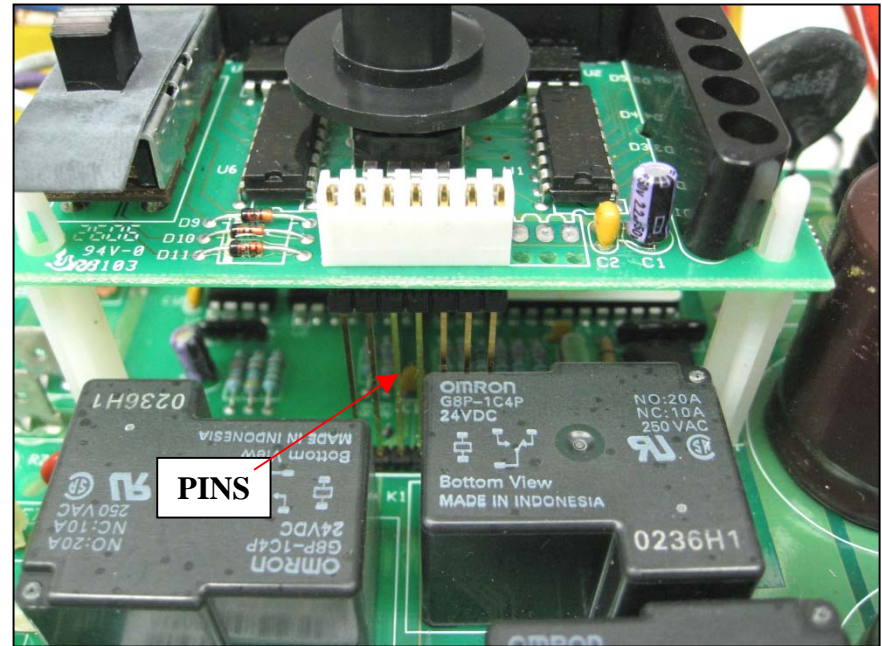


**Remove and/or reseat DSP board. Pins may be shorted together or not making contact with connector. If pins are good, check for 3 to 5 volts (DC) on pins 1 & 3, starting from the left. If DC voltage is correct, replace DSP board.**



# No LED's/LCD display

Control box shows LCD display but no LED's are illuminated.

Step I

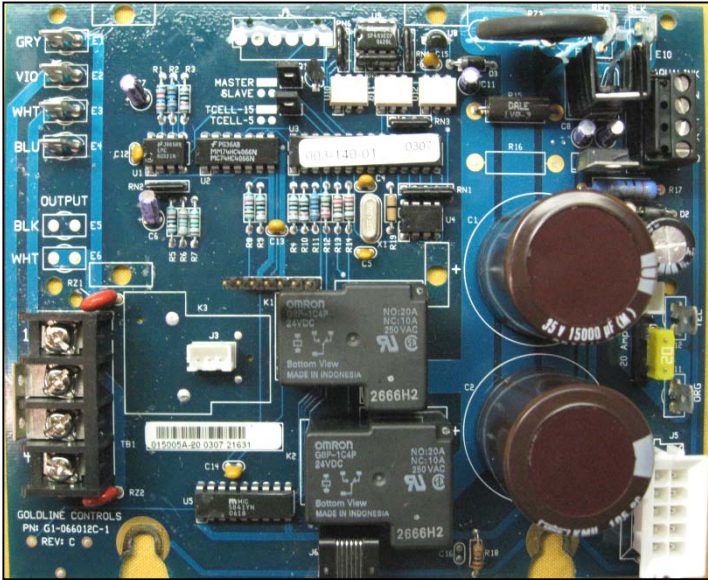

Visually inspect main PCB board for any damaged or burnt components. If damaged or burned, replace the main PCB.

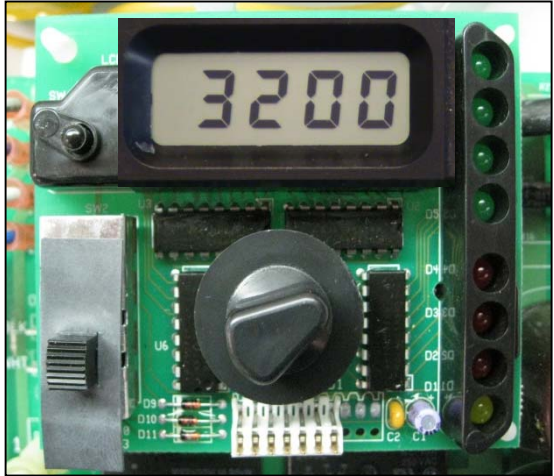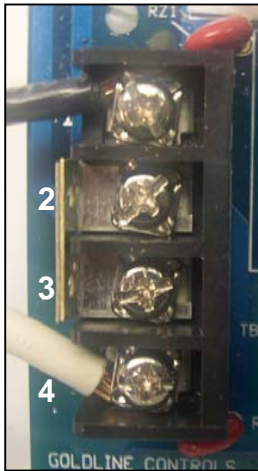


Jumpers on terminal TB1 are configured for 240 VAC (factory default), but there is 120 VAC applied to control box.

# Low/High Cell temperature

*The operating temperature range for the cell is 50° F to 140° F.*

**Verify actual water temperature**

Cell Temperature  
Sensor

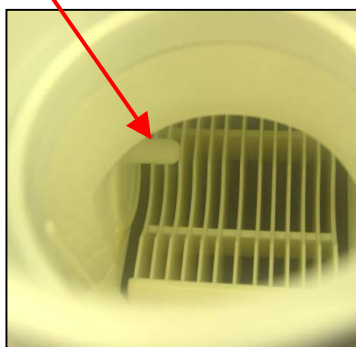

LCD display will read "COLD" when the water temperature is below 50° F  
LCD display will read "HOT" when the water temperature is above 140° F  
If the water temperature reads 215° F, the cell temperature sensor is shorted  
and the cell needs to be replaced.

**Output is scaled back to 20% at 60° F and output stops at 50° F**



# Cell Cleaning

Cell cleaning frequency is dependent on several factors; pH and calcium levels in the water are the two that have the greatest effect on how often the cell requires cleaning. Maintaining pH at the levels recommended in the Operating Instructions (7.2 - 7.8) should result in the cell being cleaned 3-4 times a year in areas with hard water. Cells may be cleaned less frequently in soft water areas.

After removing the Turbo Cell from the plumbing of your pool; inspect the cell for white deposits between the plates inside of the cell. Please remember that even if you cannot see deposits on the cell it still may need cleaning. If no deposits are found (4A), the cell may have to be held towards ample amounts of light and angled in different directions to reveal smaller white deposits deeper within the nest of the cell.



**CAUTION**

**ALWAYS ADD ACID TO WATER, NEVER WATER TO ACID. ALWAYS WEAR PROPER EYE PROTECTION AND PROTECTIVE GLOVES. USE IN A WELL VENTILATED AREA. MURIATIC AND OTHER ACIDS CAN CAUSE SEVERE INJURY, BURNS AND RESPIRATORY PROBLEMS IF NOT HANDLED PROPERLY. REFER TO THE MANUFACTURER'S DIRECTIONS FOR SAFE HANDLING.**



# Cell Cleaning Instructions

Cleaning instructions  
using a container.



We strongly recommend using a Goldline Controls cell cleaning stand. (GLX-CELLSTAND)

**Step 1:** Use a water hose to dislodge small debris.

**Step 2:** Use a non-metal (plastic or wood), non-abrasive tool to dislodge minor calcium buildup and small debris.

**Step 3:** Use a solution of water and Muriatic acid. Stand the cell vertically in the solution. Mix 1 part acid to 4 parts water. The level of the solution should be slightly over the product label. Let the cell stand in the solution for 15 minutes (Fig. 6A below), then flip the cell over and let stand on the other end (Fig. 6B below) for an additional 15 minutes. Although the cord can be submerged, be sure that the connector does not come in contact with the solution.

Inspect the cell after both sides have soaked. If there are no deposits after soaking, rinse with water and reinstall. If there are still deposits after soaking, repeat the soaking procedure until clean. The water/muriatic acid mixture can be stored for later use or it can be disposed. Follow chemical manufacturer's recommendations when storing or disposing the water/acid solution.

After you inspect the cell (and clean, if necessary) press the small "diagnostic" button next to the display for 3 seconds to stop the flashing "Inspect Cell" LED and reset the countdown timer for another 500 operational hours.



# Cell Cleaning Instructions

## Using the Goldline T-Cell Cleaning Stand


Follow the same safety and mixing instructions as described when using a container on page 14. Mix enough solution to fill the inside of the cell ( Approximately 1.5 qts). Mix 1 part acid to 4 parts water.

Fasten the cell to the T-Cell Cleaning Stand with the cord side down (Fig. 6A below). Before filling cell with muriatic acid solution, put a container underneath to avoid any spills damaging the surrounding area. Fill the cell to the top with the solution and let soak for 15 minutes (Fig. 6B below). Empty the cell and inspect. If the cell is clean, rinse with water and reinstall. If there are still deposits after soaking, repeat the soaking procedure until clean. The water/muriatic acid mixture can be stored for later use or it can be disposed of. Follow the chemical manufacturer's recommendations when storing or disposing the water/acid solution.


After you inspect the cell (and clean, if necessary) press the small "diagnostic" button next to the display for 3 seconds to stop the flashing "Inspect Cell" LED and reset the countdown timer for another 500 operational hours. If the cell was cleaned because of 'Low Salt', be sure to reset the average salt reading by following the instructions on page 4.



# Check Salt & Inspect Cell LED flashing or ON Troubleshooting Chart

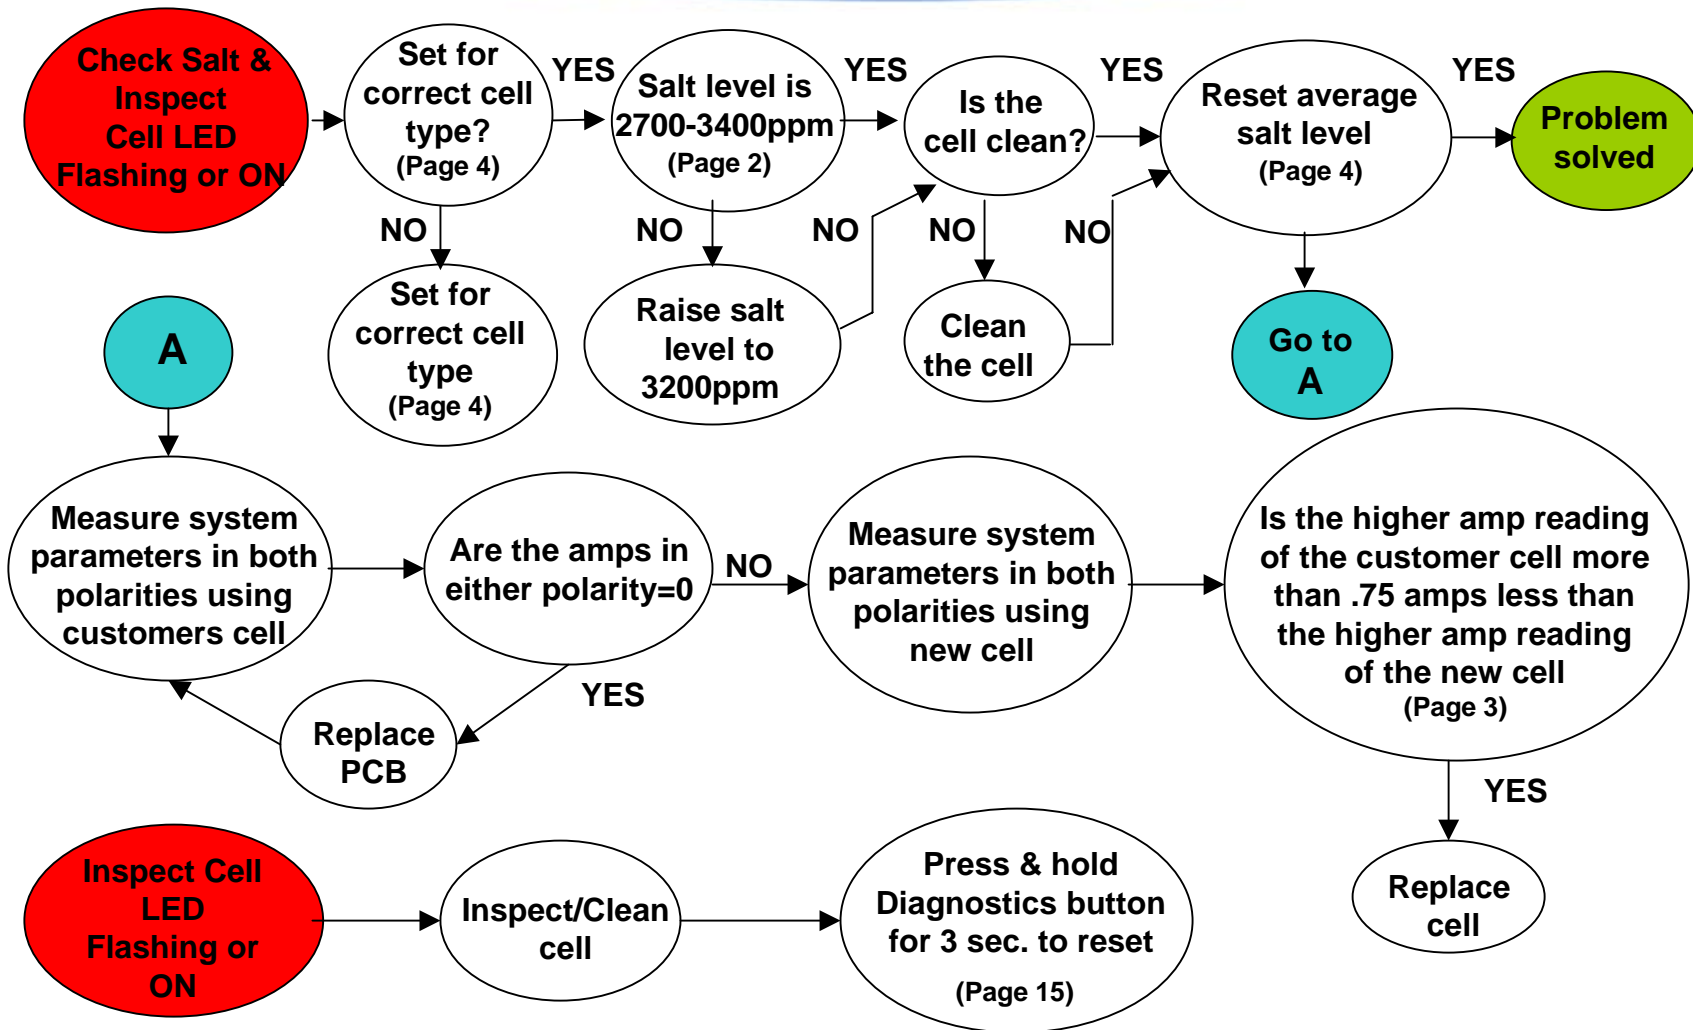


# High Salt LED ON Troubleshooting Chart

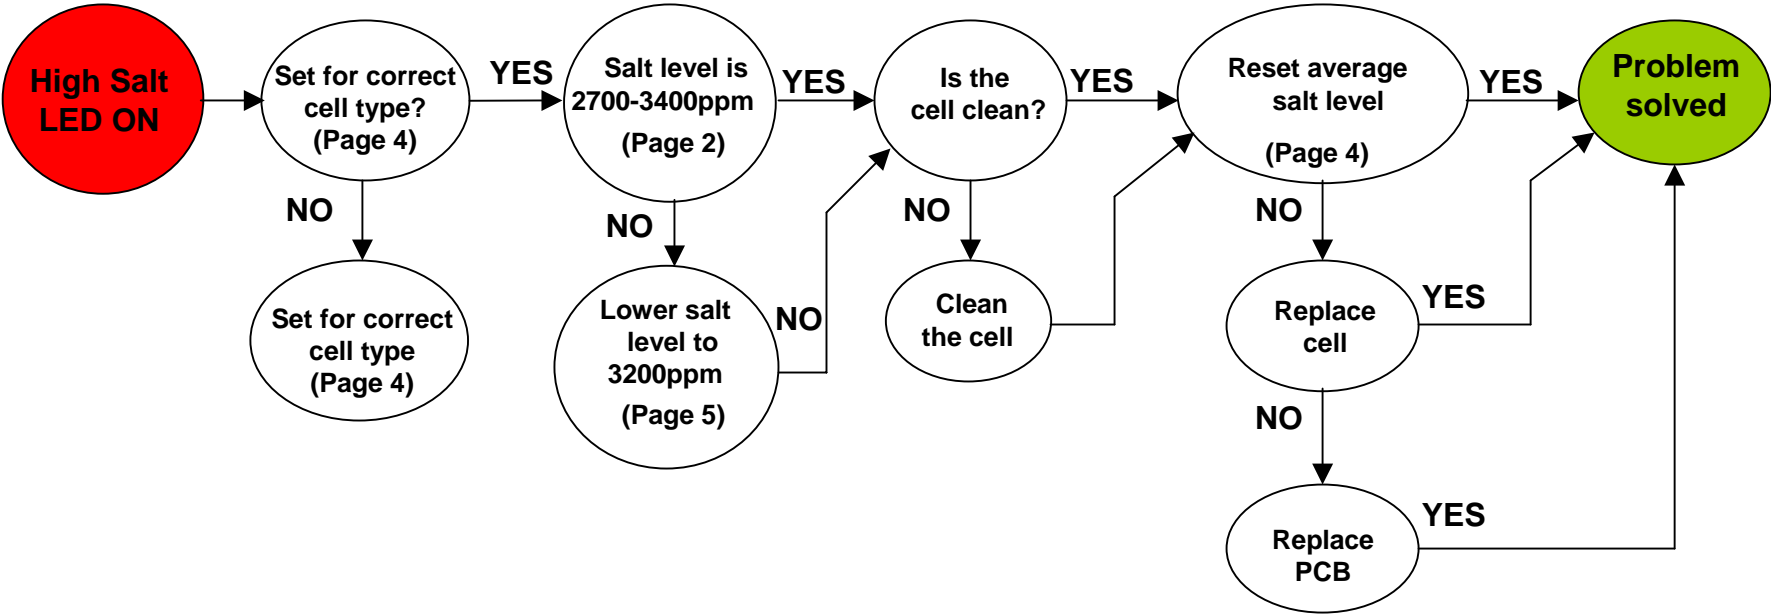





# No Flow LED Flashing Troubleshooting Chart

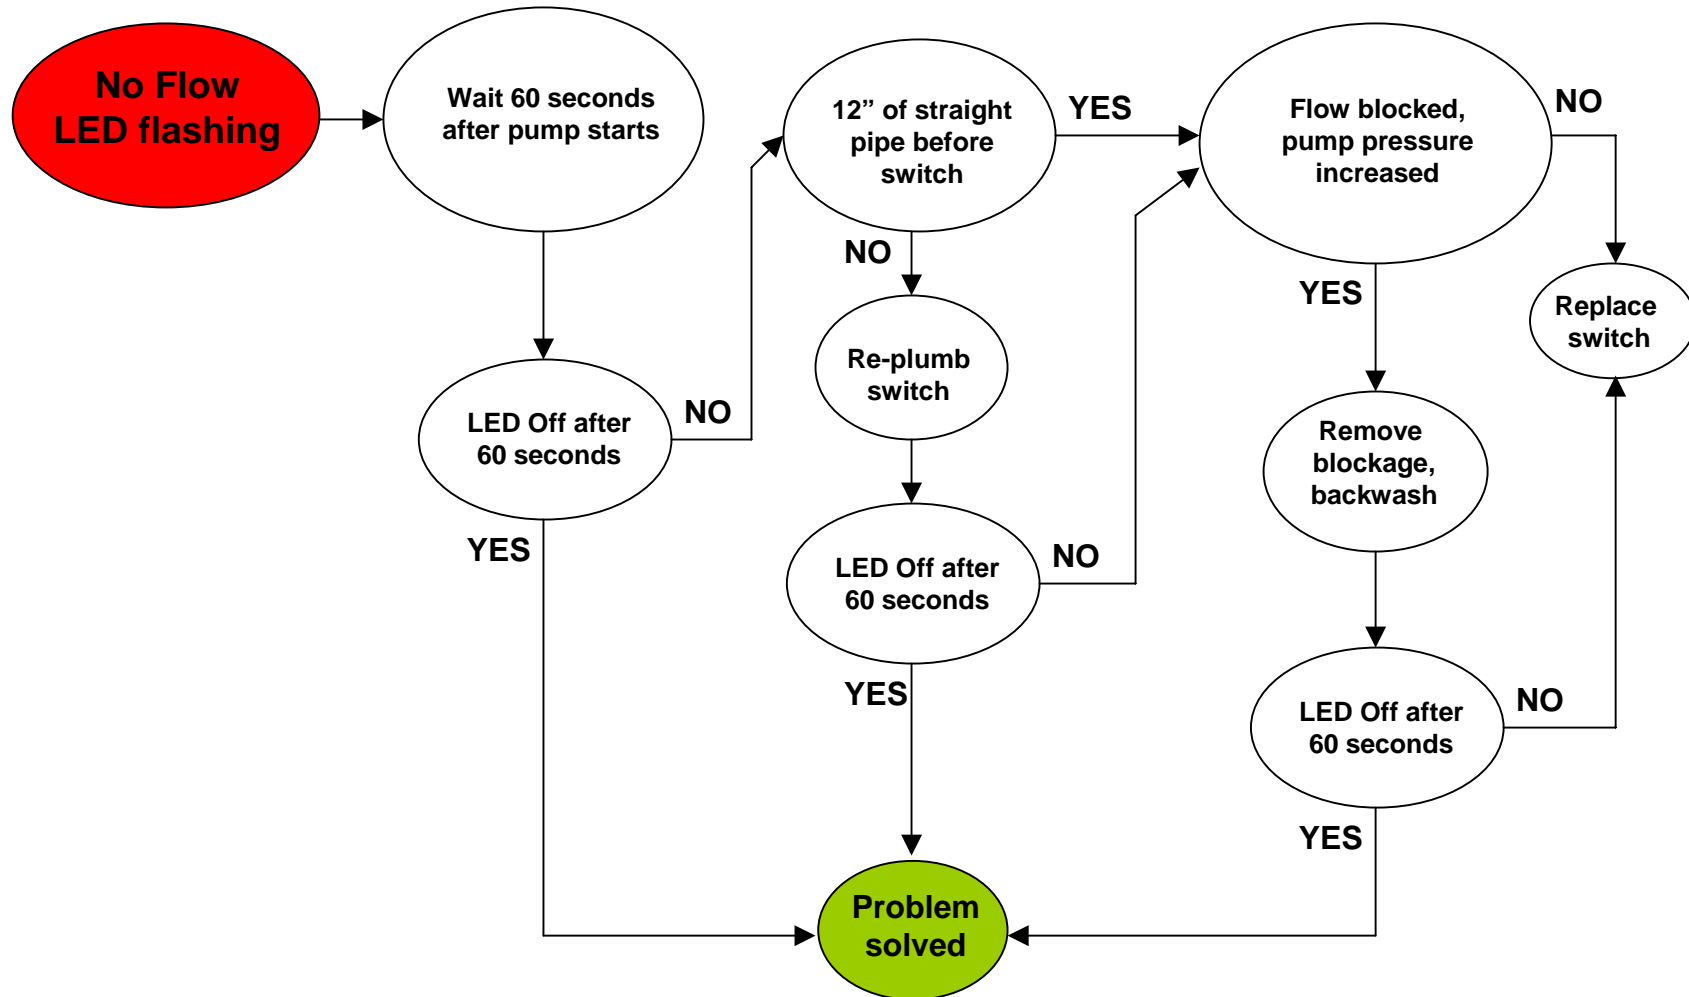

# No Flow LED ON Troubleshooting Chart

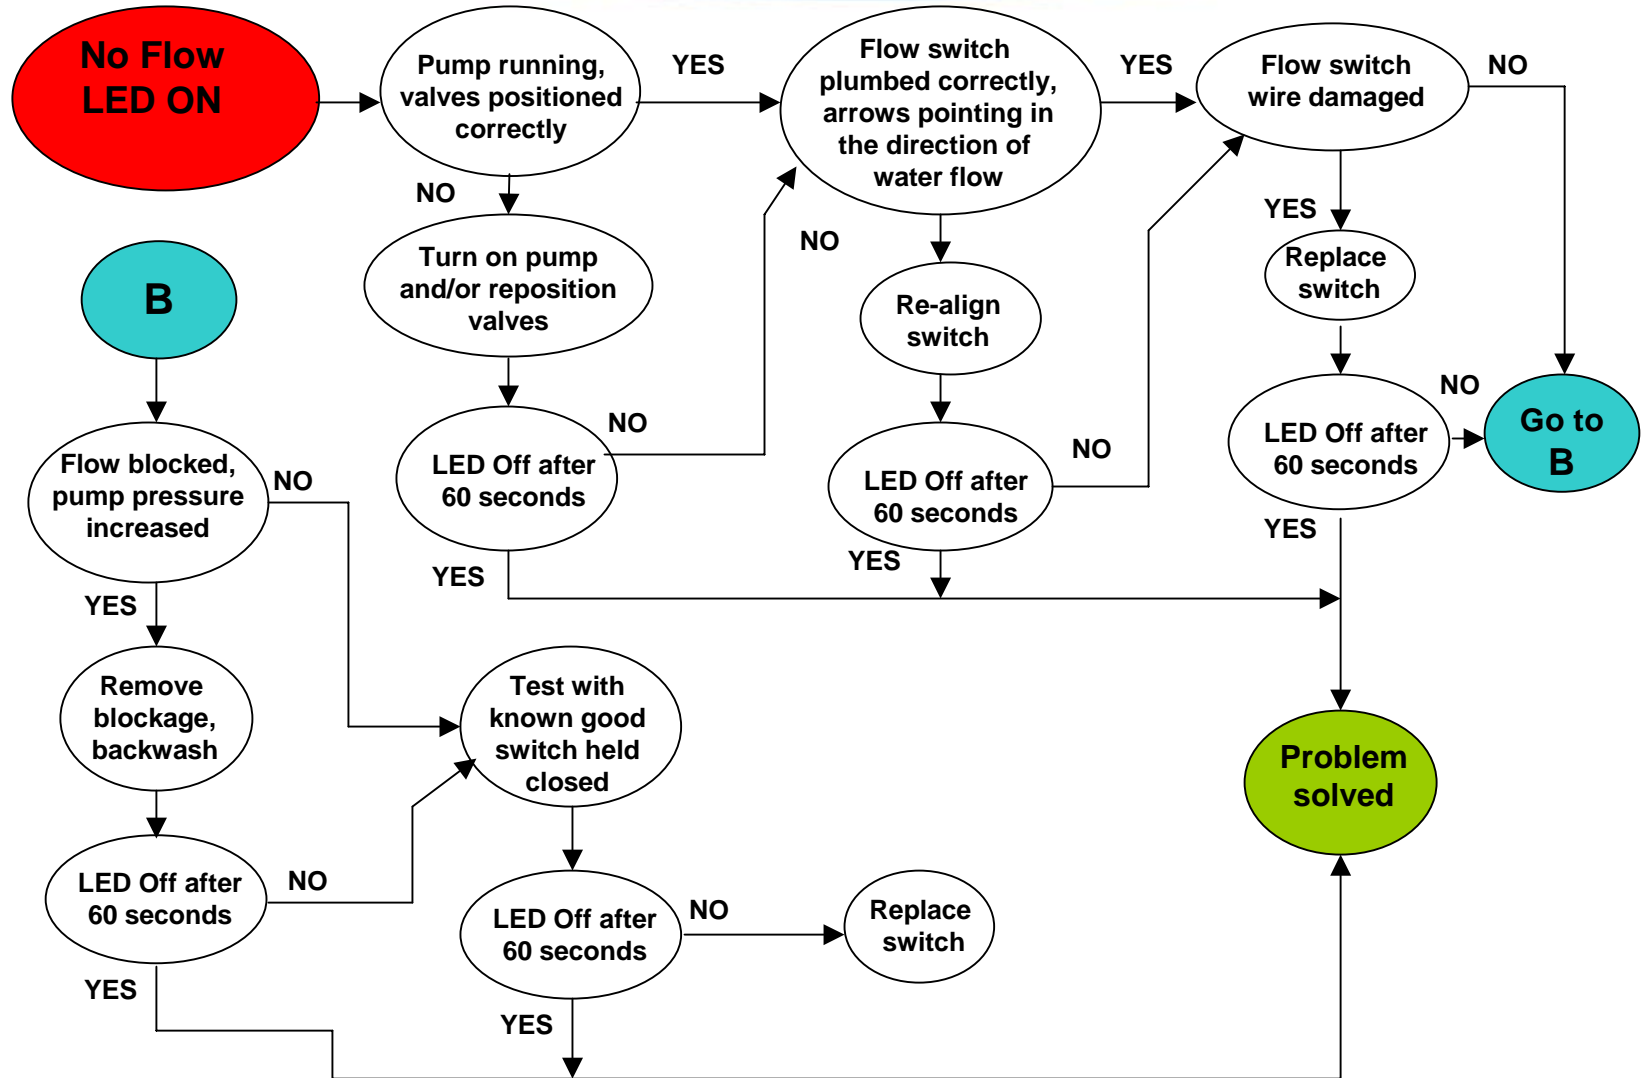

# No LED's/LCD Display Troubleshooting Chart

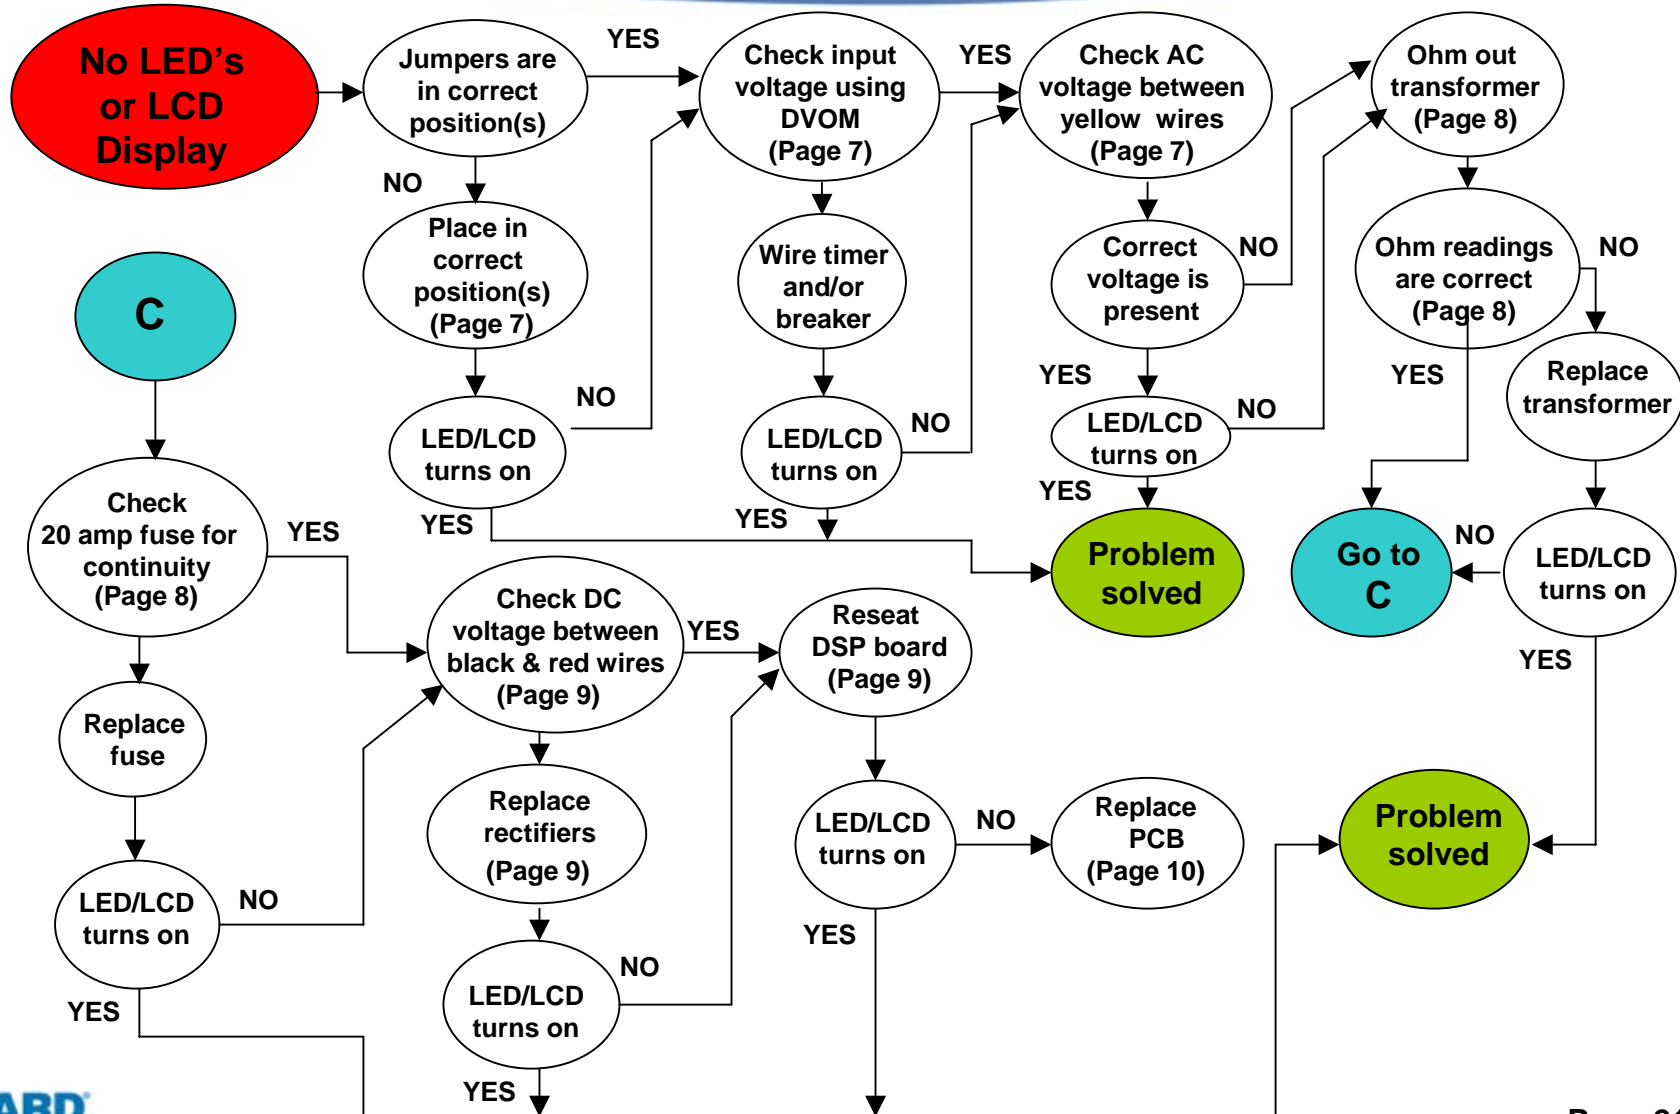

# Salt Chart

Pounds of Salt required for 3200 ppm

Current Salt Level (ppm)	Pool Size -- Gallons																
	8,000	10,000	12,000	14,000	16,000	18,000	20,000	22,000	24,000	26,000	28,000	30,000	32,000	34,000	36,000	38,000	40,000
0	213	267	320	373	427	480	533	587	640	693	747	800	853	907	960	1013	1067
200	200	250	300	350	400	450	500	550	600	650	700	750	800	850	900	950	1000
400	187	233	280	327	373	420	467	513	560	607	653	700	747	793	840	887	933
600	173	217	260	303	347	390	433	477	520	563	607	650	693	737	780	823	867
800	160	200	240	280	320	360	400	440	480	520	560	600	640	680	720	760	800
1000	147	183	220	257	293	330	367	403	440	477	513	550	587	623	660	697	733
1200	133	167	200	233	267	300	333	367	400	433	467	500	533	567	600	633	667
1400	120	150	180	210	240	270	300	330	360	390	420	450	480	510	540	570	600
1600	107	133	160	187	213	240	267	293	320	347	373	400	427	453	480	507	533
1800	93	117	140	163	187	210	233	257	280	303	327	350	373	397	420	443	467
2000	80	100	120	140	160	180	200	220	240	260	280	300	320	340	360	380	400
2200	67	83	100	117	133	150	167	183	200	217	233	250	267	283	300	317	333
2400	53	67	80	93	107	120	133	147	160	173	187	200	213	227	240	253	267
2600	40	50	60	70	80	90	100	110	120	130	140	150	160	170	180	190	200
2800	27	33	40	47	53	60	67	73	80	87	93	100	107	113	120	127	133
3000	13	17	20	23	27	30	33	37	40	43	47	50	53	57	60	63	67
3200	ideal	ideal	ideal	ideal	ideal	ideal	ideal	ideal	ideal	ideal	ideal	ideal	ideal	ideal	ideal	ideal	ideal
3400	ok	ok	ok	ok	ok	ok	ok	ok	ok	ok	ok	ok	ok	ok	ok	ok	ok
3600+	dilute	dilute	dilute	dilute	dilute	dilute	dilute	dilute	dilute	dilute	dilute	dilute	dilute	dilute	dilute	dilute	dilute

**Note: Prior to adding salt, always test water with independent tests to determine current salt and stabilizer levels.**

## How to Add Salt

Brushing the salt around will speed up the dissolving process. Do not allow the salt to sit in a pile at the bottom of the pool. Salt water is heavier than fresh water so the salt water will tend to accumulate at the deepest part of the pool. Run the filter system with the suction coming from the main drain for 24 hours to evenly distribute the salt throughout the pool.

**Note:** Allow 10-14 days for the plaster on new pools to cure before adding salt



# Software Revision Compatibility Chart

	Aqua Rite Pro	Aqua Rite	Aqua Rite XL	Aqua Trol	Aqua Logic	Aqua Plus	Pro Logic	Swimpure Plus	Swimpure Plus w/Controls	H40	SmartPure Sanitizer II	Splash CLEAR	SP40	Guardian	Nature Soft
<b>T-CELL-3 &amp; GLX-CELL-3-W</b> (pools up to 15K gallons)	1.10 or later	1.50 or later	X	None	X	X	4.10 or later	1.50 or later	4.10 or later	X	X	X	X	X	X
<b>GLX-CELL-5 &amp; GLX-CELL-5-W</b> (pools up to 20K gallons)	All revisions	1.50 or later	X	All revisions	All revisions	All revisions	All revisions	1.50 or later	All revisions	X	X	X	X	X	X
<b>T-CELL-9 &amp; GLX-CELL-9-W</b> (pools up to 25K gallons)	1.10 or later	1.50 or later	X	X	X	X	4.10 or later	1.50 or later	4.10 or later	X	X	X	X	X	X
<b>T-CELL-15 &amp; GLX-CELL-15-W</b> (pools up to 40K gallons)	All revisions	All revisions	All revisions	X	All revisions	All revisions	All revisions	All revisions	All revisions	All revisions	All revisions	All revisions	All revisions	All revisions	All revisions

# IMPORTANT !!!

## More on Chlorine Output & Salt Levels

1. The 'Desired Output %' dial on the main panel sets the level of salt cell operation as a percent of the total operating time of the entire system. A simple example is that if the pump/filter is programmed to operate a total of 8 hours in a given day and the 'Desired output %' is set to 50% the salt cell will operate (and produce chlorine) approximately half the time, or 4 hours. 50% is the factory default.
2. The salt level that is calculated (and displayed) in the system is determined from several variables. It is possible that the displayed salt level can be significantly different from the actual salt level (when measured in the water with a tester). This can happen as a result of a dirty cell or from a cell that has begun aging. Low salt should always require a cell cleaning first and then an actual meter measurement of the salt level in the water. If the cell is clean and the level of salt measured in the water is correct, then the cell has begun to age, which results in a lower calculated salt level. This is an acceptable situation, assuming the level of free chlorine in the pool is appropriate. NEVER add additional salt in this circumstance.
3. If the free chlorine is not appropriate and the steps in item 2 have been followed and addressed as needed, then the 'Desired Output %' needs to be increased in a 25% increment (for example from 50% to 75%) to allow for the salt cell to operate for a longer period (% of total operating time) in order to produce a sufficient amount of chlorine as the cell begins to age. Allow 24 hours and re-test free chlorine. Increase in increments of +10% if required. Keep in mind this is assuming the chemistry parameters are correct in the pool and there is nothing that is creating a significant chlorine demand.
4. Super-chlorinate is an additional option to use in order to 'catch up' in chlorine production when making adjustments to the desired output level. Move the switch to 'Super Chlorinate' to enable.